

CERTIFICATE

of Product Conformity (QAL1)

Certificate No.: 0000040218

Certified AMS: Model 43i for SO₂

Manufacturer: Thermo Fisher Scientific
27 Forge Parkway
Franklin, MA 02038
USA

Test Institute: TÜV Rheinland Energie und Umwelt GmbH

**This is to certify that the AMS has been tested
and found to comply with:**

**VDI 4202-1: 2002, VDI 4203-2: 2004, EN 14212: 2012,
EN 15267-1: 2009, EN 15267-2: 2009**

Certification is awarded in respect of the conditions stated in this certificate
(see also the following pages).




Publication in the German Federal Gazette
(BArz.) of 08 April 2006

This certificate will expire on:
31 March 2019

German Federal Environment Agency
Dessau, 29 April 2014

TÜV Rheinland Energie und Umwelt GmbH
Cologne, 28 April 2014

i. A. Dr. Marcel Langner



ppa. Dr. Peter Wilbring



www.umwelt-tuv.de / www.eco-tuv.com
teu@umwelt-tuv.de
Tel. +49 221 806-5200

TÜV Rheinland Energie und Umwelt GmbH
Am Grauen Stein
51105 Cologne

Accreditation according to EN ISO/IEC 17025 and certified according to ISO 9001:2008.

Certificate:

0000040218 / 29 April 2014

Test report: 936/21203248/D1 of 07 July 2006

Addendum 936/21221382/C of 20 September 2013

Initial certification: 01 April 2014

Date of expiry: 31 March 2019

Publication: BAnz AT 01 April 2014 B12, chapter VI, notification 23

Approved application

The certified AMS is suitable for continuous monitoring of SO₂ in ambient air.

The suitability of the AMS for this application was assessed on the basis of a laboratory test and a three-month field test.

The AMS is approved for a temperature range of 0 °C to +30 °C.

Any potential user should ensure, in consultation with the manufacturer, that this AMS is suitable for ambient air applications at which it will be installed.

Basis of the certification

This certification is based on:

- test report 936/21203248/D1 of 07 July 2006 of TÜV Rheinland Immissionsschutz und Energiesysteme GmbH and Addendum 936/21221382/C of 20 September 2013 of TÜV Rheinland Energie und Umwelt GmbH
- suitability announced by the German Federal Environment Agency (UBA) as the relevant body
- the on-going surveillance of the product and the manufacturing process
- publication in the German Federal Gazette (BAnz. 14 October 2006, No. 194, p. 6715, chapter IV, No. 2.2, UBA publication from 12 September 2006)
- publication in the German Federal Gazette (BAnz. 20 April 2007, No. 75, p. 4139, chapter IV, notification 1 and 6, UBA publication from 12 April 2007)
- publication in the German Federal Gazette (BAnz. 03 September 2008, No. 133, p. 3242, chapter IV, notification 13, UBA publication from 12 August 2008)
- publication in the German Federal Gazette (BAnz. 25 August 2009, No. 125, p. 2929, chapter III, notification 17, UBA publication from 03 August 2009)
- publication in the German Federal Gazette (BAnz. 28 July 2010, No. 111, p. 2597, chapter III, notification 5, UBA publication from 12 July 2010)
- publication in the German Federal Gazette (BAnz. 29 July 2011, No. 113, p. 2725, chapter III, notification 19, UBA publication from 15 July 2011)
- publication in the German Federal Gazette (BAnz. AT 20 July 2012 B11, chapter IV, notification 24, UBA publication from 06 July 2012)
- publication in the German Federal Gazette (BAnz AT 01 April 2014 B12, chapter VI, notification 23, UBA publication from 27 February 2014)

AMS designation:
SO₂ analyzer Model 43i

Manufacturer:
Thermo Electron Corporation Franklin, USA
Distribution:
Thermo Electron Corporation, Erlangen

Field of application:
For continuous monitoring of sulphur dioxide in ambient air.

Measuring ranges during the performance test:
SO₂ 0 - 700 µg/m³ und
 0 - 1000 µg/m³

Software version:
V 01.03.00.083

Testing institute:
TÜV Rheinland Immissionsschutz und Energiesysteme GmbH, Cologne,
TÜV Rheinland Group
Bericht-Nr.: 936/21203248/D of 7 July 2006

1 Notification of the German Federal Environment Agency

The new name of Thermo Electron Corp., Franklin, USA is Thermo Fisher Scientific, Franklin, USA.

Statement by TÜV Rheinland Immissionsschutz und Energiesysteme, 51101 Cologne, Germany, Dr. Peter Wilbring, dated 20th December 2006

6 Notification of announcements by the German Federal Environment Agency dated 21st February 2006 (BAnz. p. 2653) and 12th September 2006 (BAnz. p. 6715)

The measuring systems model 42i for nitrogen oxide, model 43i for sulphur dioxide, model 48i for carbon monoxide and model 49i for ozone, manufactured by Thermo Fisher Scientific, MA 02038, USA, are also manufactured and sold identically and to the same standards by MLU-Monitoring für Leben und Umwelt Ges.m.b.H., Mödling, Austria.

Statement by TÜV Rheinland Immissionsschutz und Energiesysteme, 51101 Cologne, Germany, Dr. Peter Wilbring, dated 14th December 2006

13 Notification of announcement by the German Federal Environment Agency dated 12th September 2006 (BAnz. p. 6717)

The current software version of the ambient air measuring system 43i by Thermo Fisher Scientific is:
V 01.05.06 (105721-00)

Statement by TÜV Rheinland Immissionsschutz und Energiesysteme dated 10th March 2008

17 Notification of announcement by the German Federal Environment Agency dated 12th September 2006 (BAnz. p. 6717)

The current software version of the ambient air measuring system 43i by Thermo Fisher Scientific is:
V 01.06.01 (108457-00)

Statement by TÜV Rheinland Immissionsschutz und Energiesysteme GmbH dated 1st April 2009

5 Notification of announcements by the German Federal Environment Agency dated 12th September 2006 (BAnz. p. 6717) and 3rd August 2009 (BAnz. p. 2936)

The ambient air measuring system model 43i by Thermo Fisher Scientific can now also be operated with a sample gas pump type PU1959-N86-3.07 manufactured by KNF.

Statement by TÜV Rheinland Immissionsschutz und Energiesysteme GmbH dated 23rd März 2010

19 Notification of announcements by the German Federal Environment Agency dated 12th September 2006 (BAnz. p. 6715, Chapter IV Number 2.2) and 12th July 2010 (BAnz. p. 2597, Chapter III 5th notification)

The current software version of the ambient air measuring system model 43i for SO₂ by Thermo Fisher Scientific is:

V 01.06.07 (110959-00)

Statement by TÜV Rheinland Energie und Umwelt GmbH dated 30th March 2011

24 Notification of announcements by the German Federal Environment Agency dated 12th September 2006 (BAnz. p. 6715, Chapter IV Number 2.2) and 15th July 2011 (BAnz. p. 2725, Chapter III 19th notification)

The current software version of the ambient air measuring system model 43i for SO₂ by Thermo Fisher Scientific is 01.06.08.

The ambient air measuring system model 43i for SO₂ by Thermo Fisher Scientific will be fitted with the type PU2737-N86 vacuum pump manufactured by KNF.

Statement by TÜV Rheinland Energie und Umwelt GmbH dated 20th March 2012

23 Notification of announcements by the German Federal Environment Agency dated 12th September 2006 (BAnz. p. 6717, Chapter II Number 2.2) and 6th July 2012 (BAnz. AT 20.07.2012 B11, Chapter IV 24th notification)

The measuring system model 43i for SO₂ by Thermo Fisher Scientific fulfils the requirements of Standard EN 14212 (November 2012). Furthermore, the manufacturing process and quality management system of the measuring system model 43i for SO₂ fulfil the requirements of EN 15267.

The test report of the performance test with report number 936/21203248/D1 as well as an addendum as an integral part of the test report with report number 936/21221382/C can be viewed on the internet at www.qal1.de.

The Hamamatsu 1P28HA-5 photomultiplier was withdrawn and replaced by the new Hamamatsu R11568-15 photomultiplier.

The Arcturus Bd. 101491-xx processor board was withdrawn and replaced by the new Arcturus Bd. 110570-xx processor board.

The current software version of the measuring system is:
V 02.00.00 (113419-00)

Statement by TÜV Rheinland Energie und Umwelt GmbH dated 2nd October 2013

Certified product

This certificate applies to automated measurement systems conforming to the following description:


The sample is drawn into the model 43i through the sample bulkhead. The sample flows through a hydrocarbon "kicker" which removes hydrocarbons from the sample by forcing the hydrocarbon molecules to permeate through the tube wall. The SO₂ molecules pass through the hydrocarbon "kicker" unaffected.

The sample flows into the fluorescence chamber, where pulsating UV light excites the SO₂ molecules. The condensing lens focuses the pulsating UV light into the minor assembly. The minor assembly contains four selective mirrors that reflect only the wavelength which excite SO₂ molecules.

As the excited SO₂ molecules decay to lower energy states, they emit UV light that is proportional to the SO₂ concentration. The bandpass filter allows only the wavelength emitted by the excited SO₂ molecules to reach the photomultiplier tube (PMT). The PMT detects the UV light emission from the decaying SO₂ molecules. The photo detector, located at the back of the fluorescence chamber, continuously monitors the pulsating UV light source and is connected to a circuit that compensates for fluctuations in the lamp intensity.

As the sample leaves the optical chamber, it passes through a flow sensor, a capillary, and the "shell" side of the hydrocarbon kicker. The model 43i outputs the SO₂ concentration to the front panel display, the analog outputs, and also makes the data available over the serial or ethernet connection.

The function of the pulsed fluorescence analyser, model 43i, is based on the principle that SO₂ molecules absorb ultraviolet light (UV) and are excited on a certain wavelength and then reduce to a lower energy level, whereby they emit UV light on another wavelength. The following equation applies:



In the first step, the SO₂ molecules are excited by the UV light. In the second step they return to their original condition under the emission of hν'. The intensity of the fluorescence radiation is proportional to the number of SO₂ molecules in the detection volume and thus proportional to SO₂ concentration.

The measuring principle complies with the standard reference method as stipulated in EN 14212.

General notes

This certificate is based upon the equipment tested. The manufacturer is responsible for ensuring that on-going production complies with the requirements of the EN 15267. The manufacturer is required to maintain an approved quality management system controlling the manufacture of the certified product. Both the product and the quality management systems shall be subject to regular surveillance.

If a product of the current production does not conform to the certified product, TÜV Rheinland Energie und Umwelt GmbH must be notified at the address given on page 1.

A certification mark with an ID-Number that is specific to the certified product is presented on page 1 of this certificate. This can be applied to the product or used in publicity material for the certified product is presented on page 1 of this certificate.

This document as well as the certification mark remains property of TÜV Rheinland Energie und Umwelt GmbH. With revocation of the publication the certificate loses its validity. After the expiration of the certificate and on requests of the TÜV Rheinland Energie und Umwelt GmbH this document shall be returned and the certificate mark must not be employed anymore.

The relevant version of this certificate and the validity is also accessible on the internet: qal1.de.

Certification of Model 43i for SO₂ is based on the documents listed below and the regular, continuous monitoring of the Quality Management System of the manufacturer:

Initial test:

Test report: 936/21203248/D1 of 07 July 2006
TÜV Rheinland Immissionsschutz und Energiesysteme GmbH, Cologne

Publication: BAnz. 14 Oktober 2006, No. 194, p. 6715, chapter IV, No. 2.2
Announcement by UBA from 12 September 2006

Initial certification according to EN 15267:

Certificate No. 0000040219: 29 April 2014

Expiration date of the certificate: 31 March 2019

Test report: 936/21203248/D1 of 07 July 2006
TÜV Rheinland Immissionsschutz und Energiesysteme GmbH, Cologne

Addendum 936/21221382/C of 20 September 2013
TÜV Rheinland Energie und Umwelt GmbH, Cologne

Publication: BAnz AT 01 April 2014 B12, chapter VI, notification 23
Announcement by UBA from 27 February 2014

Notification:

Publication: BAnz. 20 April 2007, No. 75, p. 4139, chapter IV, notification 1 and 6
Announcement by UBA from 12 April 2007

Publication: BAnz. 03 September 2008, No. 133, p. 3242, chapter IV, notification 13
Announcement by UBA from 12 August 2008

Publication: BAnz. 25 August 2009, No. 125, p. 2929, chapter III, notification 17
Announcement by UBA from 03 August 2009

Publication: BAnz. 28 July 2010, No. 111, p. 2597, chapter III, notification 5
Announcement by UBA from 12 July 2010

Publication: BAnz. 29 July 2011, No. 113, p. 2725, chapter III, notification 19
Announcement by UBA from 15 July 2011

Publication: BAnz AT 20 July 2012 B11, chapter IV, notification 24
Announcement by UBA from 06 July 2012

Publication: BAnz AT 01 April 2014 B12, chapter VI, notification 23
Announcement by UBA from 27 February 2014

Calculation of overall uncertainty lab test (Device 1)

Measured component:	Thermo Fisher Scientific Modell 431	Serial-No.:	Device 1
	SO2	1h-limit value:	132 nmol/mol
No.	Performance characteristic	Performance criterion	Result
1	Repeatability standard deviation at zero	$\leq 1.0 \text{ nmol/mol}$	0.230
2	Repeatability standard deviation at 1h-limit value	$\leq 3.0 \text{ nmol/mol}$	0.470
3	"lack of fit" at 1h-limit value	$\leq 4.0\% \text{ of measured value}$	-0.400
4	Sensitivity coefficient of sample gas pressure at 1h-limit value	$\leq 2.0 \text{ nmol/mol/kPa}$	0.040
5	Sensitivity coefficient of sample gas temperature at 1h-limit value	$\leq 1.0 \text{ nmol/mol/K}$	-0.080
6	Sensitivity coefficient of surrounding temperature at 1h-limit value	$\leq 1.0 \text{ nmol/mol/K}$	0.188
7	Sensitivity coefficient of electrical voltage at 1h-limit value	$\leq 0.30 \text{ nmol/mol/V}$	-0.020
8a	Interferent H ₂ O with 21 nmol/mol	$\leq 10 \text{ nmol/mol (Zero)}$	0.300
8b	Interferent H ₂ S with 200 nmol/mol	$\leq 10 \text{ nmol/mol (Span)}$	0.030
8c	Interferent NH ₃ with 200 nmol/mol	$\leq 5.0 \text{ nmol/mol (Zero)}$	1.130
8d	Interferent NO with 500 nmol/mol	$\leq 5.0 \text{ nmol/mol (Span)}$	0.530
8e	Interferent NO ₂ with 200 nmol/mol	$\leq 5.0 \text{ nmol/mol (Zero)}$	-0.600
8f	Interferent m-Xylene with 1 µmol/mol	$\leq 10 \text{ nmol/mol (Span)}$	0.770
9	Averaging effect	$\leq 7.0\% \text{ of measured value}$	-3.300
18	Difference sample/calibration port	$\leq 1.0\%$	0.000
21	Uncertainty of test gas	$\leq 3.0\%$	2.000
Combined standard uncertainty		u _c	7.1063 nmol/mol
Expanded uncertainty		U	14.2127 nmol/mol
Relative expanded uncertainty		W	10.77 %
Maximum allowed expanded uncertainty		W _{req}	15 %

Calculation of overall uncertainty lab test (Device 2)

Measured component:	Measuring device:	Serial-No.:	Device 2	132 nmol/mol
SO2	Thermo Fisher Scientific Model 43i			
		1h-limit value:		
		132 nmol/mol		
No.	Performance characteristic	Performance criterion	Result	Partial uncertainty
1	Repeatability standard deviation at zero	≤ 1.0 nmol/mol	0.130	$u_{r,z}$ 0.04
2	Repeatability standard deviation at 1h-limit value	≤ 3.0 nmol/mol	0.390	$u_{r,1h}$ 0.11
3	"lack of fit" at 1h-limit value	≤ 4.0% of measured value	-0.400	$u_{l,h}$ -0.30
4	Sensitivity coefficient of sample gas pressure at 1h-limit value	≤ 2.0 nmol/mol/kPa	0.050	u_{gp} 0.38
5	Sensitivity coefficient of sample gas temperature at 1h-limit value	≤ 1.0 nmol/mol/K	-0.210	u_{gt} -1.87
6	Sensitivity coefficient of surrounding temperature at 1h-limit value	≤ 1.0 nmol/mol/K	0.256	u_{st} 2.28
7	Sensitivity coefficient of electrical voltage at 1h-limit value	≤ 0.30 nmol/mol/V	-0.020	u_V -0.20
8a	Interferent H ₂ O with 21 nmol/mol	≤ 10 nmol/mol (Zero)	-0.470	u_{H2O} 0.02
8b	Interferent H ₂ S with 200 nmol/mol	≤ 10 nmol/mol (Span)	0.030	$u_{int, pos}$
8c	Interferent NH ₃ with 200 nmol/mol	≤ 5.0 nmol/mol (Zero)	0.530	
8d	Interferent NO with 500 nmol/mol	≤ 5.0 nmol/mol (Span)	1.230	
8e	Interferent NO ₂ with 200 nmol/mol	≤ 5.0 nmol/mol (Zero)	-1.270	
8f	Interferent m-Xylene with 1 µmol/mol	≤ 10 nmol/mol (Zero)	7.570	
9	Averaging effect	≤ 7.0% of measured value	-3.560	u_{av} -2.71
18	Difference sample/calibration port	≤ 1.0%	0.100	u_{usc} 0.13
21	Uncertainty of test gas	≤ 3.0%	2.000	u_{cg} 1.32
		Combined standard uncertainty	u_c	1.7424 nmol/mol
		Expanded uncertainty	U	7.8705 nmol/mol
		Relative expanded uncertainty	W	15.7410 %
		Maximum allowed expanded uncertainty	W_{req}	11.92 15 %

Calculation of overall uncertainty lab and field test (Device 1)

Measured component:	Measuring device:	Thermo Fisher Scientific Modell 43i	Serial-No.:	Device 1 1h-limit value: 132 nmol/mol
No.		Performance characteristic	Performance criterion	Result
1		Repeatability standard deviation at zero	\leq 1.0 nmol/mol	0.230
2	Repeatability standard deviation at 1h-limit value	\leq	3.0 nmol/mol	0.470
3	"lack of fit" at 1h-limit value	\leq 4.0% of measured value	-0.400	$u_{\text{f},\text{lh}}$ not considered, as $u_{\text{f},\text{lh}} = 0.13 < u_{\text{f}}$
4	Sensitivity coefficient of sample gas pressure at 1h-limit value	\leq 2.0 nmol/mol/kPa	0.040	u_{p} 0.30
5	Sensitivity coefficient of sample gas temperature at 1h-limit value	\leq 1.0 nmol/mol/K	-0.080	u_{gt} -0.71
6	Sensitivity coefficient of surrounding temperature at 1h-limit value	\leq 1.0 nmol/mol/K	0.188	u_{st} 1.67
7	Sensitivity coefficient of electrical voltage at 1h-limit value	\leq 0.30 nmol/mol/V	-0.020	u_{v} -0.20
8a	Interferent H ₂ O with 21 nmol/mol	\leq 10 nmol/mol (Zero)	0.300	$u_{\text{H}_2\text{O}}$ 0.02
8b	Interferent H ₂ S with 200 nmol/mol	\leq 5.0 nmol/mol (Zero)	0.030	$u_{\text{int, pos}}$ 1.130
8c	Interferent NH ₃ with 200 nmol/mol	\leq 5.0 nmol/mol (Zero)	-0.900	$u_{\text{int, pos}}$ 0.770
8d	Interferent NO with 500 nmol/mol	\leq 5.0 nmol/mol (Zero)	0.100	$u_{\text{int, neg}}$ 6.24
8e	Interferent NO ₂ with 200 nmol/mol	\leq 5.0 nmol/mol (Zero)	2.770	38.8800
8f	Interferent m-Xylene with 1 µmol/mol	\leq 10 nmol/mol (Zero)	2.030	
9	Averaging effect	\leq 7.0% of measured value	-3.300	u_{av} -2.51
10	Reproducibility standard deviation under field conditions	\leq 5.0% of average over 3 months	3.900	u_{f} 5.15
11	Long term drift at zero level	\leq 4.0 nmol/mol	0.340	$u_{\text{d,l,z}}$ 0.20
12	Long term drift at span level	\leq 5.0% of max. of certification range	2.190	$u_{\text{d,l,h}}$ 1.67
18	Difference sample/calibration port	\leq 1.0%	0.000	u_{sc} 0.00
21	Uncertainty of test gas	\leq 3.0%	2.000	u_{cg} 1.32
		Combined standard uncertainty	u_c	8.9336
		Expanded uncertainty	U	17.8671
		Relative expanded uncertainty	W	13.54
		Maximum allowed expanded uncertainty	W _{req}	15

Calculation of overall uncertainty lab and field test (Device 2)

Measured component:	Measuring device:	Thermo Fisher Scientific Model 43i	Serial-No.:	Device 2	
No.	Performance characteristic	Performance criterion	Result	Partial uncertainty	Square of partial uncertainty
1	Repeatability standard deviation at zero	≤ 1.0 nmol/mol	0.130	$u_{t,z}$ 0.04	0.0014
2	Repeatability standard deviation at 1h-limit value	≤ 3.0 nmol/mol	0.390	$u_{t,h}$ not considered, as $u_{t,h} = 0.11 < u_{r,f}$	-
3	"lack of fit" at 1h-limit value	≤ 4.0% of measured value	-0.400	$u_{t,h}$ -0.30	0.0929
4	Sensitivity coefficient of sample gas pressure at 1h-limit value	≤ 2.0 nmol/mol/kPa	0.050	$u_{g,p}$ 0.38	0.1452
5	Sensitivity coefficient of sample gas temperature at 1h-limit value	≤ 1.0 nmol/mol/K	-0.210	$u_{g,t}$ -1.87	3.4901
6	Sensitivity coefficient of surrounding temperature at 1h-limit value	≤ 1.0 nmol/mol/K	0.256	$u_{s,t}$ 2.28	5.1866
7	Sensitivity coefficient of electrical voltage at 1h-limit value	≤ 0.30 nmol/mol/V	-0.020	u_V -0.20	0.0411
8a	Interferent H ₂ O with 21 nmol/mol	≤ 10 nmol/mol (Span)	-0.470		
8b	Interferent H ₂ S with 200 nmol/mol	≤ 5.0 nmol/mol (Zero)	0.030	$u_{h,20}$ 0.02	0.0005
8c	Interferent NH ₃ with 200 nmol/mol	≤ 5.0 nmol/mol (Span)	1.230	$u_{int, pos}$	
8d	Interferent NO with 500 nmol/mol	≤ 5.0 nmol/mol (Zero)	-1.270		
8e	Interferent NO ₂ with 200 nmol/mol	≤ 5.0 nmol/mol (Span)	0.200		
8f	Interferent m-Xylene with 1 µmol/mol	≤ 5.0 nmol/mol (Zero)	-0.230	or 6.62	43.8536
9	Averaging effect	≤ 7.0% of measured value	-3.560	u_{av} -2.71	7.3608
10	Reproducibility standard deviation under field conditions	≤ 5.0% of a average over 3 months	3.900	$u_{r,f}$ 5.15	26.5019
11	Long term drift at zero level	≤ 4.0 nmol/mol	0.340	$u_{d,l,z}$ 0.20	0.0385
12	Long term drift at span level	≤ 5.0% of max. of certification range	2.700	$u_{d,l,h}$ 2.06	4.2340
18	Difference sample/calibration port	≤ 1.0%	0.100	u_{usc} 0.13	0.0174
21	Uncertainty of test gas	≤ 3.0%	2.000	u_{eq} 1.32	1.7424
Combined standard uncertainty					
Expanded uncertainty					
Relative expanded uncertainty					
Maximum allowed expanded uncertainty					

CONFIRMATION

Notification: 0000040218_00_01_rev1
on changes according to EN 15267 regarding certificate 0000040218 dated 29 April 2014

Measuring system: Model 43i for SO₂

Manufacturer: Thermo Fisher Scientific
27 Forge Parkway
Franklin, MA 02038
USA

German Federal Environmental Agency (UBA)

Announcement about the uniform practice in
monitoring emissions and ambient air.

17 July 2014
Federal Gazette BAnz AT 05.08.2014 B11

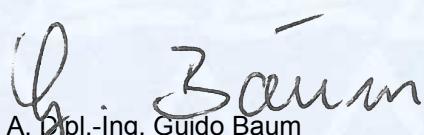
V. Notifications to the uniform practice for the continuous monitoring of
emissions and ambient air:

- 21 Notification as regards Federal Environmental Agency notices of 12 September 2006
(Federal Gazette BAnz. p. 6717, chapter II, no. 2.2) and of 27 February 2014
(Federal Gazette BAnz AT 01.04.2014 B12, chapter VI, 23rd notification)

The current software version for the Modell 43i measuring system for monitoring SO₂
manufactured by Thermo Fisher Scientific is: V 02.00.03 (114181-00)

Statement of TÜV Rheinland Energie und Umwelt GmbH of 28 March 2014

TÜV Rheinland Energie und Umwelt GmbH
Cologne, 8 September 2014


i. A. Dipl.-Ing. Guido Baum


i. A. Dipl. Ing. Carsten Röllig

www.umwelt-tuv.de
teu@umwelt-tuv.de
Tel. +49 221 806-5200

TÜV Rheinland Energie und Umwelt GmbH
Am Grauen Stein
51105 Cologne

<p>Test institute accredited to EN ISO/IEC 17025:2005 by DAkkS (German Accreditation Body). This accreditation is limited to the accreditation scope defined in the enclosure to the certificate D-PL-11120-02-00.</p>
--

CONFIRMATION

Notification: 0000040218_00_02_rev1
on changes according to EN 15267 regarding certificate 0000040218 dated 29 April 2014

Measuring system: Modell 43i for SO₂

Manufacturer: Thermo Fisher Scientific
27 Forge Parkway
Franklin, MA 02038
USA

German Federal Environmental Agency (UBA)

Announcement about the uniform practice in
monitoring emissions and ambient air.
25 February 2015
Federal Gazette BAnz AT 02 April 2015 B5

IV. Notifications to the uniform practice for the continuous monitoring of emission and ambient air:

- 17 Notification as regards Federal Environment Agency (UBA) notices of 12 September 2006 (Federal Gazette (BAnz.) p. 6715, chapter IV number 2.2) and of 17 July 2014 (Federal Gazette (BAnz) AT 05 August 2014 B11, chapter V 21th notification)

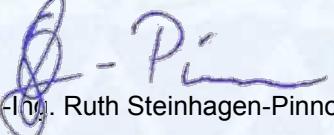
The current software version for the Model 43i measuring system for SO₂ manufactured by Thermo Fisher Scientific, is:

V 02.02.00 (114619-00)

Statement of TÜV Rheinland Energie und Umwelt GmbH of 22 September 2014

TÜV Rheinland Energie und Umwelt GmbH
Cologne, 30. April 2015

i. A. Dipl.-Ing. Ruth Steinhagen-Pinnow


www.umwelt-tuv.de
teu@umwelt-tuv.de
Tel. +49 221 806-5200

i. A. Dipl. Ing. Carsten Röllig


TÜV Rheinland Energie und Umwelt GmbH
Am Grauen Stein
51105 Cologne

Test institute accredited to EN ISO/IEC 17025:2005 by DAkkS (German Accreditation Body. This accreditation is limited to the accreditation scope defined in the enclosure to the certificate D-PL-11120-02-00.)	
---	--

CONFIRMATION

Notification: 0000040218_00_03
on changes according to EN 15267 regarding certificate 0000040218_00 dated 29 April 2014

Measuring system: Modell 43i for SO₂

Manufacturer: Thermo Fisher Scientific
27, Forge Parkway
Franklin, MA 02038
USA

German Federal Environmental Agency (UBA)

**Announcement about the uniform practice in
monitoring emissions and ambient air
dated 14 March 2016
Federal Gazette: BAnz AT 14.03.2016 B7**

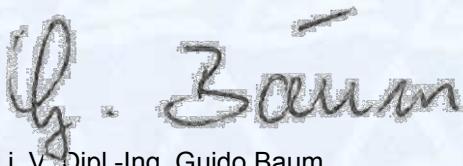
- V. Notifications to the uniform practice for the continuous monitoring of emission and ambient air:
- 13 Notification as regards Federal Environment Agency (UBA) notices of 12 September 2006 (BAnz. p. 6715, chapter IV number 2.2) and of 25 February 2015 (BAnz AT 02.04.2015 B5, chapter IV notification 17)

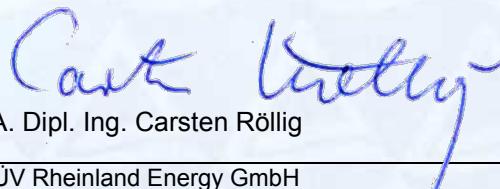
The current software version of the measuring equipment Model 43i for SO₂ of Thermo Fisher Scientific is:

V 02.02.07

Statement of TÜV Rheinland Energie und Umwelt GmbH of 22 October 2015

TÜV Rheinland Energy GmbH
Cologne, 26 April 2016


i. V. Dipl.-Ing. Guido Baum


i. A. Dipl. Ing. Carsten Röllig

www.umwelt-tuv.eu tre@umwelt-tuv.eu Tel. +49 221 806-5200	TÜV Rheinland Energy GmbH Am Grauen Stein 51105 Cologne
--	---

Test institute accredited to EN ISO/IEC 17025:2005 by DAkkS (German Accreditation Body).
This accreditation is limited to the accreditation scope defined in the enclosure to the certificate D-PL-11120-02-00.

CONFIRMATION

Notification: 0000040218_00_04
on changes according to EN 15267 regarding certificate 0000040218_00 dated 29 April 2014

Measuring system: model 43i measuring system for SO₂

Manufacturer: Thermo Fisher Scientific
27 Forge Parkway
Franklin, MA 02038
USA

German Federal Environmental Agency (UBA)

**Announcement about the uniform practice in
monitoring emissions and ambient air
dated 14 July 2016**
Federal Gazette: BAnz AT 01.08.2016 B11

- V. Notifications to the uniform practice for the continuous monitoring of emission and ambient air:
- 37 Notification as regards Federal Environmental Agency (UBA) notices of 12 September 2006 (BAnz. p. 6715, chapter IV number 2.2) and of 18 February 2016 (BAnz AT 14.03.2016 B7, chapter V 13th notification)

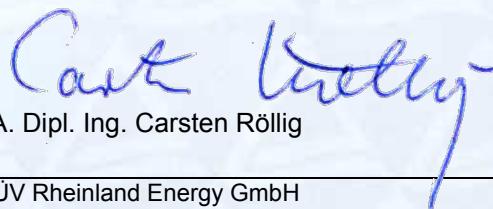
The current software version of the model 43i measuring system for SO₂ manufactured by Thermo Fisher Scientific is:
V 02.02.08

Supply of the optical lens used for this measuring system is ensured by two different suppliers.

Statement issued by TÜV Rheinland Energy GmbH dated 27 May 2016.

TÜV Rheinland Energy GmbH
Cologne, 18 August 2016


i. V. Dipl.-Ing. Guido Baum


i. A. Dipl. Ing. Carsten Röllig

www.umwelt-tuv.eu tre@umwelt-tuv.eu Tel. +49 221 806-5200	TÜV Rheinland Energy GmbH Am Grauen Stein 51105 Cologne
--	---

Test institute accredited to EN ISO/IEC 17025:2005 by DAkkS (German Accreditation Body).
This accreditation is limited to the accreditation scope defined in the enclosure to the certificate D-PL-11120-02-00.